

Oxygen sensors made by monolayer graphene under room temperature

C. W. Chen, S. C. Hung, M. D. Yang, C. W. Yeh, C. H. Wu, G. C. Chi, F. Ren, and S. J. Pearton

Citation: [Applied Physics Letters](#) **99**, 243502 (2011); doi: 10.1063/1.3668105

View online: <http://dx.doi.org/10.1063/1.3668105>

View Table of Contents: <http://scitation.aip.org/content/aip/journal/apl/99/24?ver=pdfcov>

Published by the [AIP Publishing](#)

Articles you may be interested in

[Effects of Ga ion-beam irradiation on monolayer graphene](#)

Appl. Phys. Lett. **103**, 073501 (2013); 10.1063/1.4818458

[Terahertz and optical study of monolayer graphene processed by plasma oxidation](#)

Appl. Phys. Lett. **102**, 131901 (2013); 10.1063/1.4795526

[Detection of organic vapors by graphene films functionalized with metallic nanoparticles](#)

J. Appl. Phys. **112**, 114326 (2012); 10.1063/1.4768724

[Monolayer graphene film/silicon nanowire array Schottky junction solar cells](#)

Appl. Phys. Lett. **99**, 133113 (2011); 10.1063/1.3643473

[Probing nanoscale conductance of monolayer graphene under pressure](#)

Appl. Phys. Lett. **99**, 013110 (2011); 10.1063/1.3609317

The advertisement features a dark blue background with a subtle grid pattern. At the top left, the text 'NEW! Asylum Research MFP-3D Infinity™ AFM' is written in white and orange. Below this, the phrase 'Unmatched Performance, Versatility and Support' is written in orange. On the right side, the Oxford Instruments logo is displayed, consisting of the word 'OXFORD' in a large, white, serif font above the word 'INSTRUMENTS' in a smaller, white, sans-serif font, all enclosed in a white rectangular box. Below the logo is the tagline 'The Business of Science®'. The central part of the advertisement is filled with four images: a blue and white textured surface, a brown and orange textured surface, a yellow and orange textured surface, and a white and blue textured surface. Each image is accompanied by a short text description: 'Stunning high performance', 'Simpler than ever to GetStarted™', 'Comprehensive tools for nanomechanics', and 'Widest range of accessories for materials science and bioscience'. At the bottom right, there is a photograph of the MFP-3D Infinity AFM instrument, which is a white and blue device with a large, flat, rectangular sample stage.

Oxygen sensors made by monolayer graphene under room temperature

C. W. Chen,¹ S. C. Hung,^{2,a)} M. D. Yang,³ C. W. Yeh,³ C. H. Wu,³ G. C. Chi,⁴ F. Ren,⁵ and S. J. Pearton⁶

¹Department of physics, National Central University, Jhong-Li 320, Taiwan

²Optical Science Center, National Central University, Jhong-Li 320, Taiwan

³Institute of Nuclear Energy Research, P. O. Box 3-11, Lungtan 32500, Taiwan

⁴Department of Photonics, National Chiao Tung University, Hsinchu 300, Taiwan

⁵Department of Chemical Engineering, University of Florida, Gainesville, Florida 32611, USA

⁶Department of Material Science and Engineering, University of Florida, Gainesville, Florida 32611, USA

(Received 23 September 2011; accepted 18 November 2011; published online 13 December 2011)

The electrical resistivity of monolayer graphene exhibit significant changes upon expose to different concentration of oxygen (O₂) at room temperature. The monolayer graphene, grown by chemical vapor deposition with perfect uniformity within 1 cm × 1 cm will attach O₂ molecules and enhance the hole conductivity, which will lead to a change of resistivity of graphene thin film. We quantified the change of resistivity of graphene versus different O₂ concentration and the detection limit of the simple O₂ sensor was 1.25% in volume ratio. © 2011 American Institute of Physics. [doi:10.1063/1.3668105]

Oxygen gas (O₂) is widely used in a lot of applications such as medical,¹ life support and recreational use,^{2,3} industrial, and scientific area.^{4,5} However, oxygen gas can be toxic at elevated partial pressures, leading to convulsions and other health problems. Oxygen toxicity usually begins to occur at partial pressures more than 50 kPa or 2.5 times the normal sea-level O₂ partial pressure of about 21 kPa (equal to about 50% oxygen composition at standard pressure). On the other hand, highly concentrated sources of oxygen promote rapid combustion. Fire and explosion hazards exist when concentrated oxidants and fuels are brought into close proximity; however, an ignition event, such as heat or a spark, is needed to trigger combustion. Oxygen itself is not the fuel, but the oxidant. Combustion hazards also apply to compounds of oxygen with a high oxidative potential, such as peroxides, chlorates, nitrates, perchlorates, and dichromates because they can donate oxygen to a fire.

Recently, graphene and graphene oxide play important roles in a lot of areas of chemistry, physics, biochemical, and material science because of its excellent electrical and crystal properties.^{6–10} As well known, graphene is composed of honeycomb lattice structures of carbon atoms arranged via sp² bonds. The delocalizes pi(π) bonds of graphene allow charge carriers to have zero rest mass and high mobility,^{11,12} which is approximately three one-thousandths of the speed of light. Gas sensing is one of the promising applications for graphene.^{13,14} High surface-to-volume ratio in conjunction with high conductivity translates into high sensitivity to molecular disruption on the graphene surface.¹⁵

There were lots of articles published to show that the potential of graphene and graphene oxide as gas sensors. Graphene oxide reduced by hydrazine was used to detect H₂ and CO by Arsat *et al.*;¹⁶ NO₂, NH₃, and di-nitro-toluene by Fowler *et al.* With mechanically exfoliated graphene,¹⁷ Dan *et al.* detected H₂O, NH₃, octanoic acid, and trimethylamine,¹⁸

while Schedin *et al.* experimented with NO₂, H₂O, I₂, NH₃, CO, and ethanol.¹⁹ Tour *et al.* using graphene nanoribbons to detect O₂ with very high sensitivity.²⁰

In this letter, we demonstrate a low cost, easily fabricated oxygen sensor using a monolayer graphene grown by chemical vapor deposition (CVD) with simply in Ohmic contact in two corners. We quantified the sensitivity, the temporal resolution, and the limit of detection of these sensors for O₂ detection.

The monolayer graphene used for the O₂ sensing were grown on 25 μm thick copper foil in a quartz tube furnace system using a CVD method involving methane and hydrogen gases. Under vacuum conditions of 10 mTorr, the furnace would be heated with a 2 sccm flow of H₂ present. The growth temperatures was 1000 °C. After 40 min of heating to allow the copper foil to anneal, a flow of 35 sccm of methane would be introduced for a growth time ranging from 30 s to 15 min. A quick cooling method was used (~300 °C/min) after growth, and the methane and hydrogen gas flows were continued throughout the cooling process. The graphene films on copper were then characterized using scanning electron microscopy (SEM) images. After transferring the films to Si/SiO₂ wafers through polymethyl methacrylate (PMMA) coating and iron (III) nitrate etching, the films would be further analyzed by Hall measurement and Raman spectroscopy.

Figure 1 shows the SEM images of graphene on copper foil where the Cu grains are clearly visible. A continuously graphene thin film was observed because we can see clearly the Cu surface steps and graphene wrinkles.

Raman spectroscopy was used to evaluate the quality and uniformity of graphene on a SiO₂/Si substrate. Figure 2 shows the Raman spectra and maps of the D and 2D bands providing information on the defect density and film thickness. The thickness and uniformity of the graphene films were evaluated via color contrast under optical microscope and Raman spectra. The Raman spectrum in Fig. 2(a) show typical features of monolayer graphene: (1) a ~0.5 G-to-2D

^{a)}Author to whom correspondence should be addressed. Electronic mail: shengchun@ufl.edu.

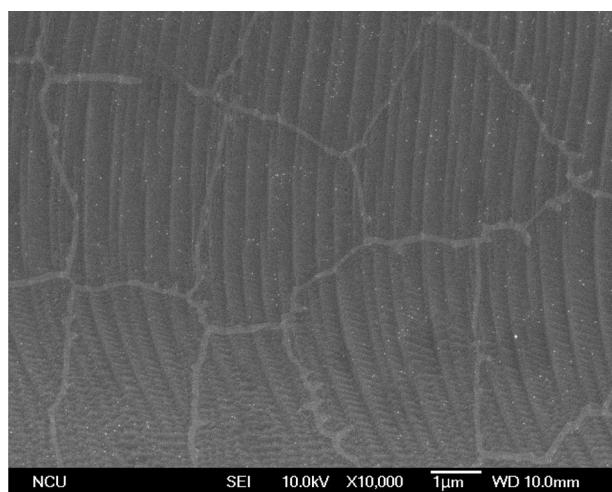


FIG. 1. SEM images of graphene on copper foil.

intensity ratio and (2) a symmetric 2D band centered at $\sim 2680\text{ cm}^{-1}$ with a full width at half maximum of $\sim 26\text{ cm}^{-1}$. As shown in Figs. 2(b) and 2(c), the 2D and the G maps clearly show the presence of more than one layer in the flakes. An analysis of the intensity of the optical image over the whole sample (1 cm by 1 cm) showed that the area with the lightest pink color is more than 95%, and all Raman spectra randomly collected from this area show uniformly monolayer graphene was transferred on SiO₂/Si substrate.

For the O₂ sensing measurement, the sensor was mounted on a carrier and put in a gas chamber filled by N₂ gas. The temperature of chamber was kept at room temperature and a constant forward bias voltage of 500 mV was applied to the Ohmic contacts of the sensor. Finally, different amounts of O₂ gas were injected into the chamber. Figure 3

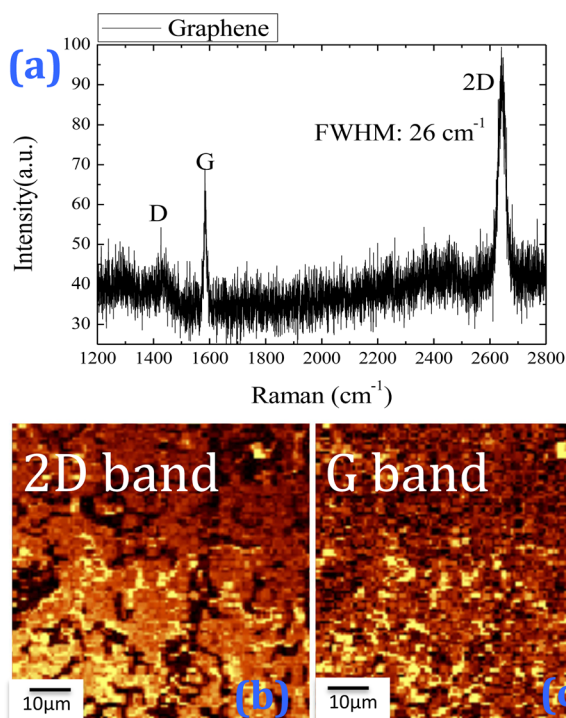
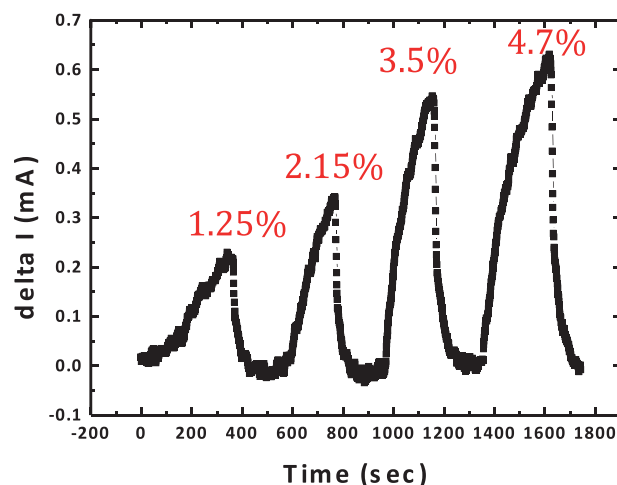
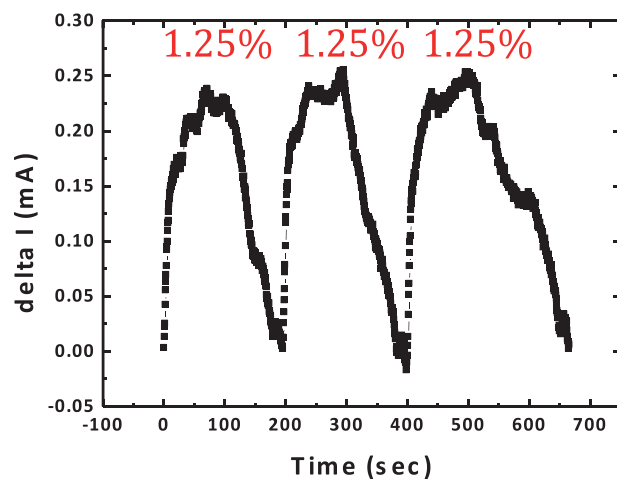


FIG. 2. (Color online) (a) Raman spectrum of monolayer of graphene. (b) Raman mapping of 2D band. (c) Raman mapping of G band.

FIG. 3. (Color online) Real time O₂ detection with different concentration using graphene on SiO₂/Si substrate.

shows the real time O₂ detection with graphene on SiO₂/Si. The current of the sensor showed a rapid increase when the O₂ concentration was changed to 1.25% volume ration in the open cavity with continuous gas flow. A further increase in the current for the sensor was observed when the O₂ concentration increased to 4.7% volume ratio. These abrupt current increases were due to the change in charges in the graphene upon a shift in O₂ concentration. The sensing mechanism of O₂ on graphene is because when O₂ molecules were attached on the graphene thin films and it will act as a p-type dopants. As described by Fowler *et al.* in his recently research results (Ref. 17), residual epoxide and carboxylic groups expected in chemically produced graphene are electron-withdrawing and promote some holes into the conduction band. So, when the O₂ molecules were attached on the graphene thin film and they will enhance the hole conduction and generate a significant decrease in resistance.

The O₂ sensor showed a good repeatability, as illustrated in Figure 4; the current response of the graphene sensor to O₂ gas flow rate was switching from 0% to 1.25% volume ratio. The change in current for the sensor exposed between 0 ppm to 400 ppm was still considerably larger than the

FIG. 4. (Color online) Real time O₂ detection with the same concentration using graphene on SiO₂/Si substrate.

background noise. Thus, graphene sensors could be used to detect small difference in O₂ concentration.

In conclusion, graphene sensor showed rapid change in the current when exposed to different O₂ concentration ambient at room temperature. These results show the potential of graphene for O₂ sensing applications.

This work was supported by the National Science Council of Taiwan under grant number NSC 100-2112-M-009-018.

- ¹M. A. Sim, P. Dean, J. Kinsella, R. Black, R. Carter, and M. Hughes, *Anaesthesia* **63**(9), 938 (2008).
- ²G. W. Morgenthaler, D. A. Fester, and C. G. Cooley, *Acta Astronaut.* **32**(1), 39 (1994).
- ³J. T. Webb, R. M. Olson, R. W. Krutz, G. Dixon, and P. T. Barnicott, *Aviat., Space Environ. Med.* **60**(5), 415 (1989).
- ⁴E. Hand, *Nature* **452**(7185), 259 (2008).
- ⁵J. R. Miller, M. Berger, L. Alonso, Z. Cerovic, Y. Goulas, S. Jacquemoud, J. Louis, G. Mohammed, I. Moya, R. Pedros, J. F. Moreno, W. Verhoef, and P. J. Zarco-Tejada, presented at International Geoscience and Remote Sensing Symposium (IGARSS) 2003.
- ⁶S. Stankovich, D. A. Dikin, G. H. B. Dommett, K. M. Kohlhaas, E. J. Zimney, E. A. Stach, R. D. Piner, S. T. Nguyen, and R. S. Ruoff, *Nature* **442**, 282 (2006).
- ⁷S. Watcharotone, *Nano Lett.* **7**, 1888 (2007).

- ⁸C.-A. Di, D. Wei, G. Yu, Y. Liu, Y. Guo, and D. Zhu, *Adv. Mater.* **20**, 3289 (2008).
- ⁹X. Wang, L. Zhi, and K. Mullen, *Nano Lett.* **8**, 323 (2007).
- ¹⁰H. A. Becerill, J. Mao, Z. Liu, R. M. Stoltenberg, Z. Bao, and Y. Chen, *ACS Nano* **2**, 463 (2008).
- ¹¹K. V. Emtsev, A. Bostwick, K. Horn, J. Jobst, G. L. Kellogg, L. Ley, J. L. McChesney, T. Ohta, S. A. Reshanov, J. Rohrl *et al.*, *Nature Mater.* **8**, 203 (2009).
- ¹²K. S. Novoselov, A. K. Geim, S. V. Morozov, D. Jiang, M. I. Katsnelson, I. V. Grigorieva, S. V. Dubonos, and A. A. Firsov, *Nature* **438**, 197 (2005).
- ¹³F. Schedin, A. K. Geim, S. V. Morozov, E. W. Hill, P. Blake, M. I. Katsnelson, and K. S. Novoselov, *Nature Mater.* **6**, 652 (2007).
- ¹⁴J. T. Robinson, F. K. Perkins, E. S. Snow, Z. Q. Wei, and P. E. Sheehan, *Nano Lett.* **8**, 3137 (2008).
- ¹⁵R. Van Noorden, *Chemistry World* (Royal Society of Chemistry, Cambridge, UK, 2008), Vol. 5, p. 56.
- ¹⁶R. Arsat, M. Breedon, M. Shafiei, P. G. Spizziri, S. Gilje, R. B. Kaner, K. Kalan-tar-Zadeh, and W. Wlodarski, *Chem. Phys. Lett.* **467**, 344 (2009).
- ¹⁷J. D. Fowler, M. J. Allen, V. C. Tung, Y. Yang, R. B. Kaner, and B. H. Weiller, *ACS Nano* **3**, 301 (2009).
- ¹⁸Y. P. Dan, Y. Lu, N. J. Kybert, Z. T. Luo, and A. T. C. Johnson, *Nano Lett.* **9**, 1472 (2009).
- ¹⁹F. Schedin, A. K. Geim, S. V. Morozov, E. W. Hill, P. Blake, M. I. Katsnelson, and K. S. Novoselov, *Nature Mater.* **6**, 652 (2007).
- ²⁰S. S. Rao, A. Stesmans, K. Keunen, D. V. Kosynkin, A. Higginbotham, and J. M. Tour, *Appl. Phys. Lett.* **98**, 083116 (2011).