

A Novel 16-Channel Wireless System for Electroencephalography Measurements With Dry Spring-Loaded Sensors

Lun-De Liao, Shang-Lin Wu, Chang-Hong Liou, Shao-Wei Lu, Shi-An Chen, Sheng-Fu Chen, Li-Wei Ko, and Chin-Teng Lin, *Fellow, IEEE*

Abstract—Understanding brain function using electroencephalography (EEG) is an important issue for cerebral nervous system diseases, especially for epilepsy and Alzheimer’s disease. Many EEG measurement systems are used reliably to study these diseases, but their bulky size and the use of wet sensors make them uncomfortable and inconvenient for users. To overcome the limitations of conventional EEG measurement systems, a wireless and wearable multichannel EEG measurement system is proposed in this paper. This system includes a wireless data acquisition device, dry spring-loaded sensors, and a size-adjustable soft cap. We compared the performance of the proposed system using dry versus conventional wet sensors. A significant positive correlation between readings from wet and dry sensors was achieved, thus demonstrating the performance of the system. Moreover, four different features of EEG signals (i.e., normal, eye-blinking, closed-eyes, and teeth-clenching signals) were measured by 16 dry sensors to ensure that they could be detected in real-life cognitive neuroscience applications. Thus, we have shown that it is possible to reliably measure EEG signals using the proposed system. This paper presents novel insights into the field of cognitive neuroscience, showing the possibility of studying brain function under real-life conditions.

Index Terms—Dry sensor, electroencephalography (EEG), electroencephalography measurement system, size-adjustable soft cap, wireless data acquisition device.

I. INTRODUCTION

STUDYING brain function has become an important issue in neuroscience [1]–[3]. The electroencephalography (EEG) imaging technique is important for probing brain activation, and it is the most widely used technique in both basic neuroscience research [4]–[6] and clinical applications [7], [8]. With the increased use of EEG, the requirements for EEG data acquisition devices [9] and signal processing methods have become more stringent [10]–[12]. The EEG-based brain-computer interface (BCI) [13] system provides a reliable and efficient means of communication between users and computers. This system has recently been introduced for neuroscience [5] and rehabilitation engineering [14] applications, including motor imagery [15]–[19], drowsiness detection [20], [21], and sleep analysis [22], [23].

Current EEG systems are not sized appropriately for real-life use, as their bulky size and wiring limitations restrict the available range of BCI experiments and the corresponding applications. In addition, conventional wet sensors are often used for EEG measurements, but these sensors require preparation of the skin or the application of conductive electrolytes at the skin-sensor interface, which can be time-consuming and uncomfortable for the user. Moreover, the conductive gel may cause a short circuit between nearby sensors when it is applied excessively, and in cognitive experiments, drying of the conductive gel in wet sensors can result in poor readings.

To overcome the limitations of conventional wet sensors, such as skin preparation, different types of dry sensors have been developed [24]–[32]. Some of these dry sensors are based on micro-electromechanical systems (MEMS) [26], [29], [30], [32], which acquire the EEG signals from the forehead [29]. There are several drawbacks using dry MEMS sensors, including the high manufacturing cost and the hard substrate, which is uncomfortable to wear. Other types of dry sensors are made using fabric-based sensors [33], [34], which are a more comfortable option than dry MEMS sensors. However, fabric-based sensor measurements are not suitable for use on hairy sites (i.e., parietal and occipital sites). Until now, dry sensors integrated with wearable and wireless EEG systems have not been available.

Manuscript received June 27, 2012; revised September 3, 2012; accepted October 29, 2012. Date of publication January 9, 2014; date of current version May 8, 2014. This work was supported in part by the UST-UCSD International Center of Excellence in Advanced Bioengineering, which is sponsored by the Taiwan National Science Council I-RiCE Program under Grant NSC-100-2911-I-009-101 and Grant NSC-101-2911-I-009-101; in part by the Aiming for the Top University Plan of National Chiao Tung University, the Ministry of Education, Taiwan, under Grant 101W963; in part by the National Science Council of Taiwan under Contract NSC-100-2321-B-009-003; in part by the VGHUST Joint Research Program, Tsou’s Foundation, Taiwan, under Contract VGHUST101-G5-2-1; and in part by the Army Research Laboratory through Cooperative Agreement under Grant W911NF-10-2-0022. The Associate Editor coordinating the review process was Dr. Wendy Van Moer.

L.-D. Liao is with the Singapore Institute for Neurotechnology, National University of Singapore, Singapore 119077, and also with the Brain Research Center, National Chiao Tung University, Hsinchu 300, Taiwan.

S.-L. Wu, C.-H. Liou, and S.-W. Lu are with the Institute of Electrical Control Engineering, National Chiao Tung University, Hsinchu 300, Taiwan.

S.-A. Chen is with the Brain Research Center, National Chiao Tung University, Hsinchu 300, Taiwan.

S.-F. Chen is with the National Health Research Institutes, Miaoli 350, Taiwan.

L.-W. Ko is with the Brain Research Center, National Chiao Tung University, Hsinchu 300, Taiwan, and also with the Department of Biological Science and Technology, National Chiao Tung University, Hsinchu 300, Taiwan.

C.-T. Lin is with the Brain Research Center, National Chiao Tung University, Hsinchu 300, Taiwan, and also with the Institute of Electrical Control Engineering, National Chiao Tung University, Hsinchu 300, Taiwan (e-mail: ctklin@mail.nctu.edu.tw).

Color versions of one or more of the figures in this paper are available online at <http://ieeexplore.ieee.org>.

Digital Object Identifier 10.1109/TIM.2013.2293222

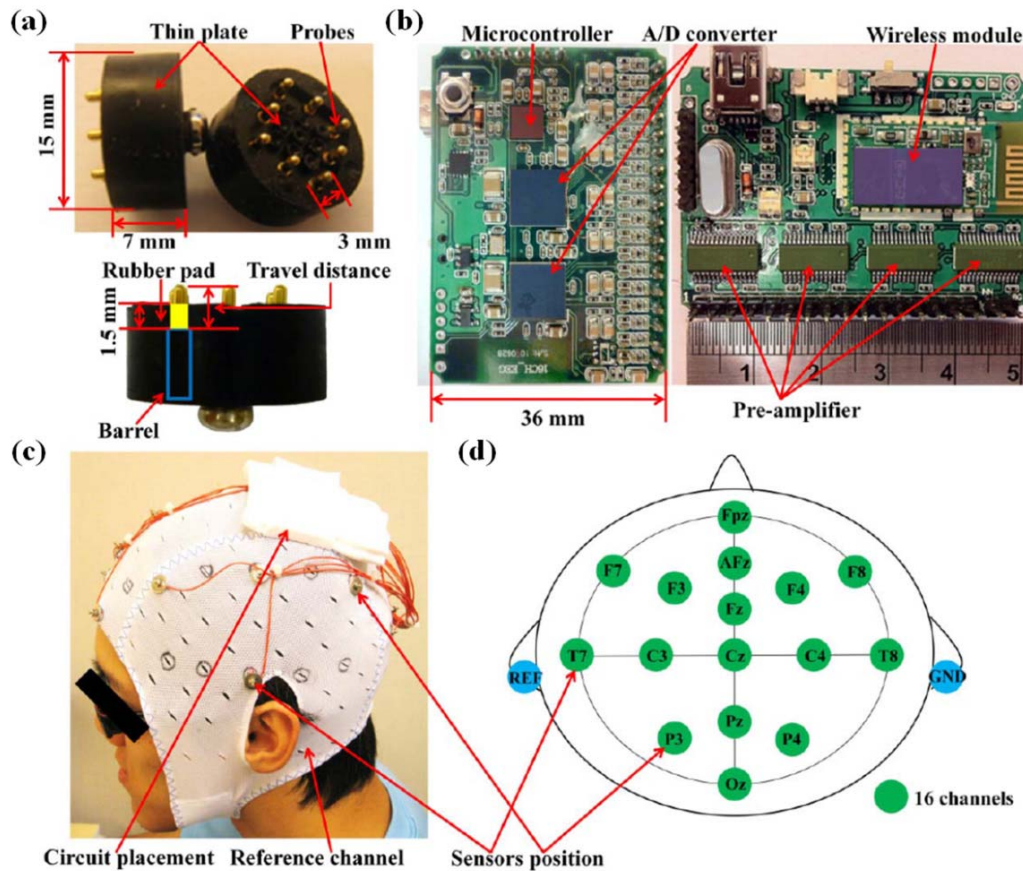


Fig. 1. Proposed design for the 16-channel EEG system with dry sensors. (a) Dry EEG sensor with a 15 mm diameter, a 7 mm depth and 8 probes. The travel distance of each probe is 3 mm. There is a unique rubber pad around the bottom surface of the sensors. (b) Wireless EEG acquisition system with a preamplifier, an ADC, a microcontroller, and a wireless module. Each circuit board is 36 mm in width. (c) Size-adjustable soft cap with 16 dry EEG sensors. The placement of each sensor is in accordance. (d) Standard 10-20 EEG system.

In this paper, a wearable, wireless 16-channel EEG system with dry sensors was developed, consisting of dry spring-loaded sensors, a wireless acquisition system and a size-adjustable wearable soft cap. The dry sensors can be utilized without the application of a conductive gel, even on hairy sites. The sensors provide good electrical conductivity for effective acquisition of EEG signals. In contrast to traditional EEG measurement systems that use dry sensors, the proposed system requires reduced skin preparation and benefits from highly accurate EEG signals. Thus, the wireless and wearable EEG measurement system developed here has the potential to be used in cognitive engineering applications [35].

II. MATERIALS AND METHODS

The fundamental components of the proposed system are shown in Fig. 1(a)–(d), including the dry spring-loaded sensors, a wireless EEG acquisition system, and a size-adjustable wearable soft cap, all in accordance with the international 10–20 system for sensor placements [35].

A. Design of Dry Spring-Loaded Sensor

The dry spring-loaded sensors were designed with eight probes, as shown in Fig. 1(a). These probes were

designed to contact the skin and maintain electrical conduction: they are coated with gold on all surfaces to establish an electrical contact similar to that of conventional wet sensors. Building on our design from a previous paper [36], here, we propose the addition of a unique rubber pad around the bottom surface of the sensors, as indicated in Fig. 1(a). This pad can significantly reduce the pain when force is applied on the sensors. To test and demonstrate this design, a dry sensor composed of the probes, a spring, a plunger, a barrel, and the rubber pad was constructed. The top of the probe has a spheroid shape and is coated with gold to enhance the conductivity. Gold is chemically stable, biocompatible, and does not easily react with other substances. Moreover, gold's high conductivity, high resistance to oxidation and resistance to environmental degradation (i.e., resistance to other non-chlorinated acids) justify the extensive use of gold materials in the electronics and biomedical industries. The spring force of the sensor was ~ 23 g, which is the level required for EEG signal measurements on the scalp [36]. Depending on the location of spring contact with the scalp, the spring could either increase or decrease in length.

In contrast to conventional wet sensors, dry sensors exhibit the electronic characteristics of electrically conductive materials. They obtain high-quality signals without skin abrasion or

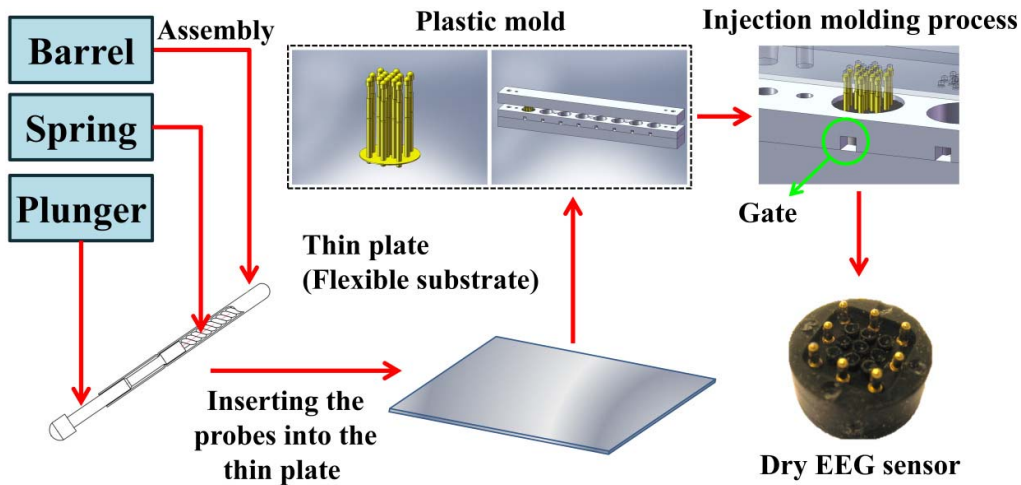


Fig. 2. Assembly process for the dry sensors, including injection-molding and packaging processes.

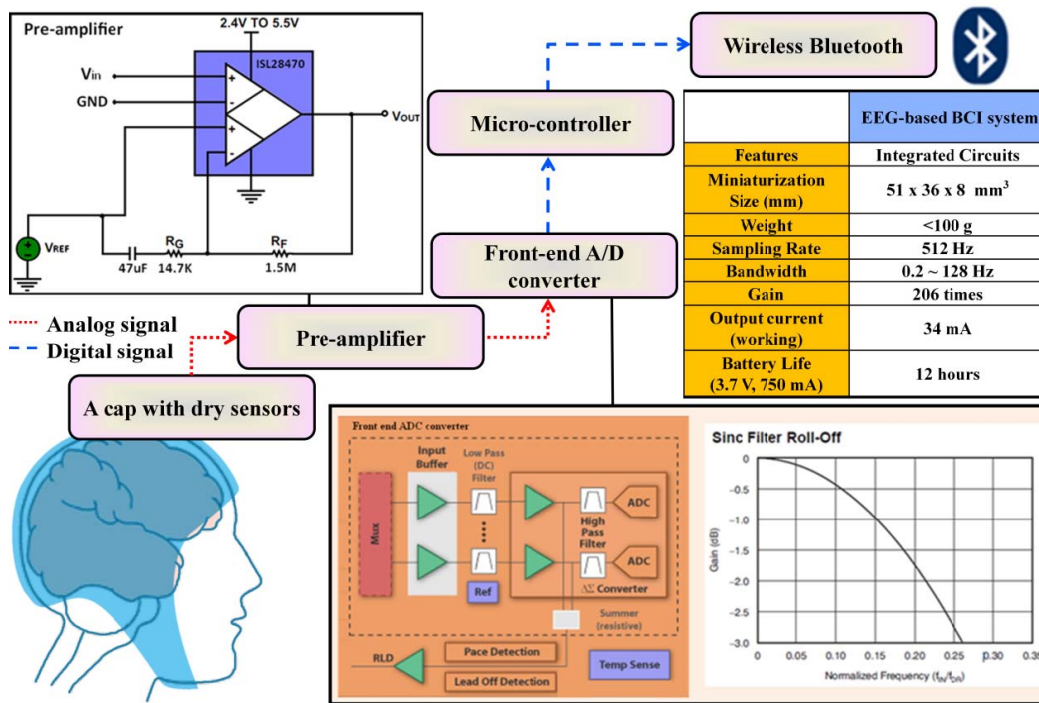


Fig. 3. Wireless and wearable 16-channel EEG system with dry sensors.

preparation. Moreover, unlike fabric-based sensors [37], [38], the spring-loaded sensors allow a high level of geometric conformity between the sensor and the irregular scalp surface due to the flexibility of the probes when applied to the scalp. This flexibility also can increase the skin-sensor contact area on hairy sites.

B. Manufacturing of Dry EEG Sensors

The manufacturing process for the dry EEG sensors is shown in Fig. 2. Eight probes are inserted into a piece of thin copper plating that is applied to the flexible base of the sensor. After insertion, the eight probes on the copper plate are all conductive. When force is applied to the sensor, the flexible substrate permits high geometric conformity to the irregular

scalp surface. The spring provides buffering effects, enabling the dry EEG sensor to contact the scalp when force is applied. The flexibility of the spring increases the comfort when the sensor contacts the scalp. After fabricating and inserting the probes into the flexible substrate, an injection-molding process is used to integrate the flexible base with several probes. The probes with the elastic base are fixed into the plastic mold. Similar to the thin plate and spring contact probes, the sensors also remain flexible after the injection molding process [36].

C. EEG Acquisition Module

A typical EEG signal ranges from 10 to 100 μV in amplitude when measured from the scalp. EEG signals measured through sensors on the scalp are easily affected by

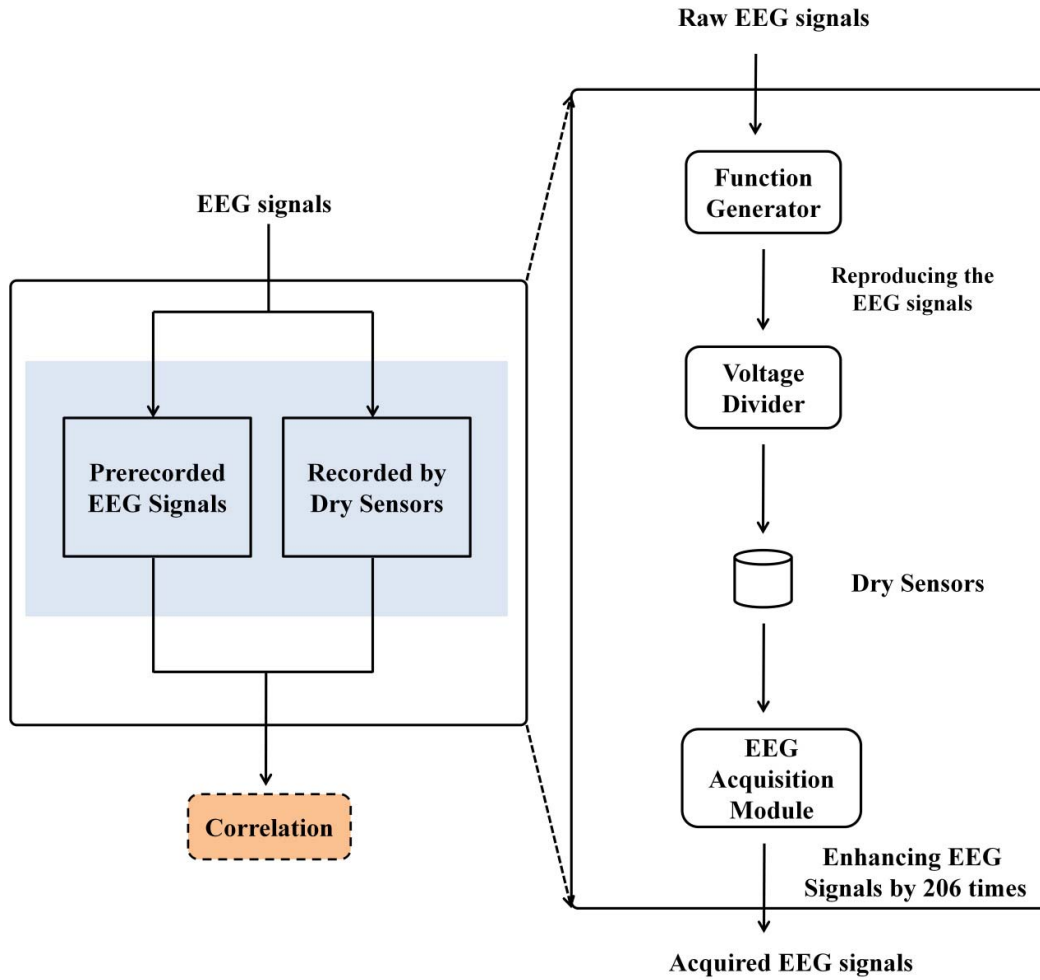


Fig. 4. Testing the accuracy of the signal from the dry sensors.

artifacts indirectly related to brain activation [39], [40], such as electromyography and electrooculography. These artifacts are irrelevant physiological signals in this experiment and may significantly obscure the EEG signals of interest. The 16-channel EEG acquisition module was designed to measure true EEG signals, as shown in Fig. 1(b). The acquisition module consists of four major units: 1) a preamplifier unit; 2) a front-end analog-to-digital converter (ADC) unit; 3) a microcontroller unit; and 4) a wireless unit. The wireless 16-channel integrated circuit-based acquisition module described here measures approximately $51 \times 36 \times 8 \text{ mm}^3$ and can be embedded into our system. When measured by the dry EEG sensors, EEG signals are first amplified by the preamplifier unit (ISL28470, Intersil, USA), which amplifies the voltage difference between the reference and EEG electrodes and simultaneously rejects common-mode noise (i.e., power line noise). An instrumentation amplifier was used as the preamplifier because of its extremely high input impedance and high common-mode rejection ratio (CMRR). The instrumentation amplifier improves the CMRR and amplifies the EEG signals such that microvolt-level signals can be detected successfully.

The gain of the preamplifier unit is set to 103 V/V, and the cut-off frequency is regulated to 0.2 Hz by a high-pass

filter. The transfer function of this preamplifier circuit is as follows:

$$V_{\text{out}} = \left(1 + \frac{R_F}{R_G + 1/sC}\right) V_{\text{in}} \quad (1)$$

$$\frac{V_{\text{out}}}{V_{\text{in}}} = \left(1 + \frac{R_F}{R_G + 1/sC}\right) \quad (2)$$

$$\frac{V_{\text{out}}}{V_{\text{in}}} = \left(1 + \frac{R_F}{R_{\text{eq}}}\right) = \left(1 + \frac{1.5 \times 10^6}{14.7 \times 10^3 + 1/j\omega \times 47 \times 10^{-6}}\right). \quad (3)$$

The preamplifier circuit, shown in Fig. 3, has two amplifiers: one that is connected to the input voltage (V_{in}) and the ground and another that is connected to the feedback of V_{out} and reference voltage (V_{REF}). Thus, using the superposition theorem [41], [42], the transfer function of the preamplifier circuit is as shown in (1). The values of the transfer function (e.g., $R_F = 1.5 \text{ M}\Omega$, $R_G = 14.7 \text{ K}\Omega$ and equivalent impedance of $47 \text{ }\mu\text{F}$) are shown in (2). Equation (2) can be reorganized into the form of a high-pass filter with input signals of frequency ω , as presented in (3). The high-pass filter is regulated to 0.2 Hz and consists of a resistor (resistance R_G) and a capacitor connected in series. Therefore, the gain of the preamplifier unit is 103 V/V [i.e., $(1 + 1.5 \times 10^6/14.7 \times 10^3)$].

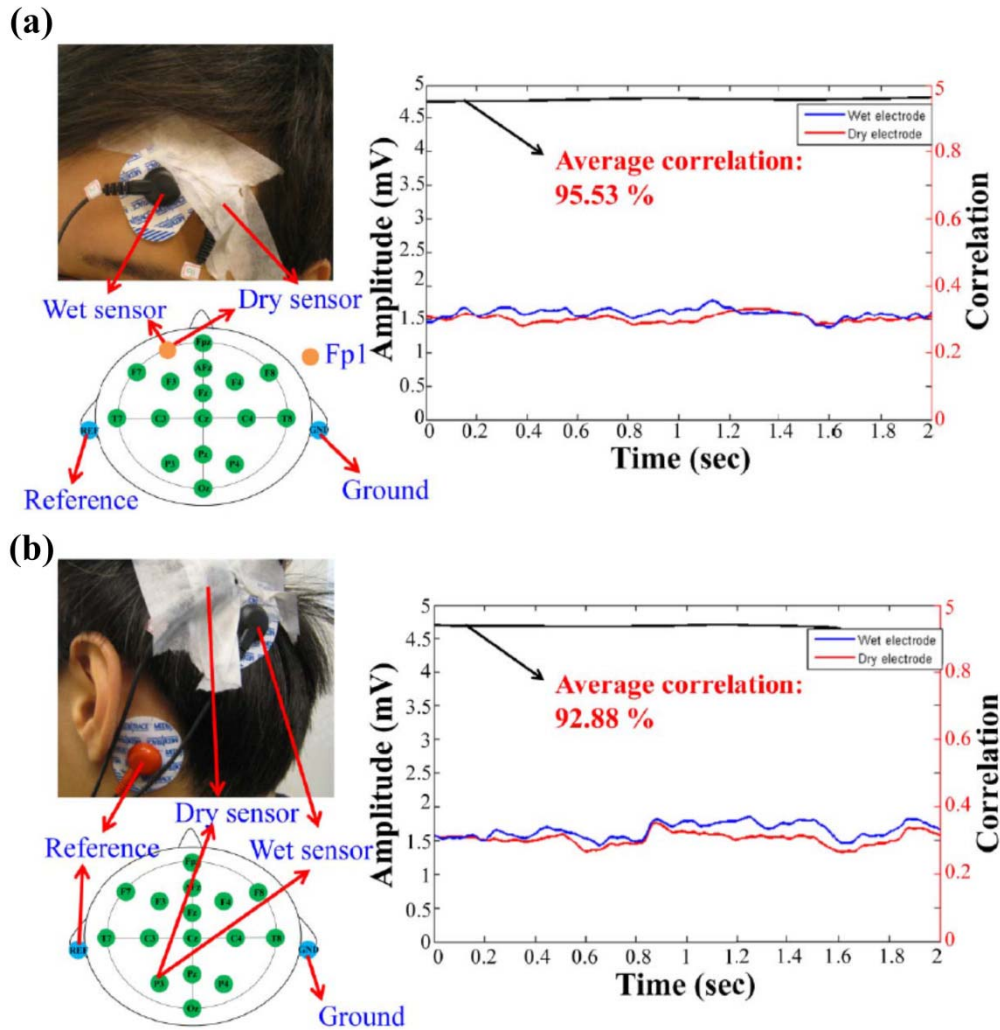


Fig. 5. Comparison of the signal quality between the dry and wet sensors. EEG measurements from (a) frontal sites (Fp1) and (b) hairy sites (P3) are shown.

The front-end ADC (ADS1298, Texas Instruments, USA) is used to digitize the amplified EEG signal. The minimum input voltage of the ADC ranges from -1.94 to 1.94 mV, and the maximum ranges from -23.30 to 23.30 mV. The least significant bit voltage is $0.286 \mu\text{V}$. The simplified design of this system reduces the space requirements and power consumption compared to other systems. The front-end ADC digitizes the analog EEG signals with a sampling rate of 512 Hz, and a sinc filter removes the frequencies above 128 Hz, as shown in Fig. 3. The microcontroller unit (MSP430F5522, Texas Instruments) was used to regulate the signal sampling rate, magnification, and noise reduction. The processed EEG signal from the ADC was reduced to 60 Hz noise by the microcontroller unit using a moving average. The microcontroller unit set the default gain of the ADC unit to 2 V/V. Therefore, the total gain of the EEG signal was set to 206 V/V (i.e., 103×2 V/V). Adjusting the gain of the ADC unit to the maximum ($12 \times$), the total gain of the EEG signal is 1236 V/V (i.e., 103×12 V/V). After removing the noise and amplifying the EEG signal, the EEG signal was transmitted to the computer interface by a wireless module, specifically a Bluetooth module (HL-MD08R-C2, HotLife

Electronic Technology Co., Ltd., Taiwan). The Bluetooth module supports a high band-width transmission with its high baud rate (i.e., $921\,600$ b/s), according to the Bluetooth v2.1+ enhanced data rate specification. Power for the board is supplied by a commercial 750 mAh Li-ion battery with a 3 V output voltage, which can also supply power for the EEG acquisition circuit and can be continuously operated for over 12 h.

D. BCI System

Standard EEG systems have multiple channels (i.e., 64 or 128 channels) available for measuring brain activity, with sensors organized on an elastic head cap according to the international $10-20$ [43] system. Such a cap is suitable only if the sensors are covered with a conductive gel. To solve this problem, an easy-to-use, size-adjustable soft cap with dry sensors is proposed here. The EEG size-adjustable soft cap is fitted with 16 dry sensor sites, as shown in Fig. 1(c). The cap is composed of an elastic material, providing a more comfortable fit and more flexibility, enabling the experimenter to place the sensors in close contact with the user's scalp, which is

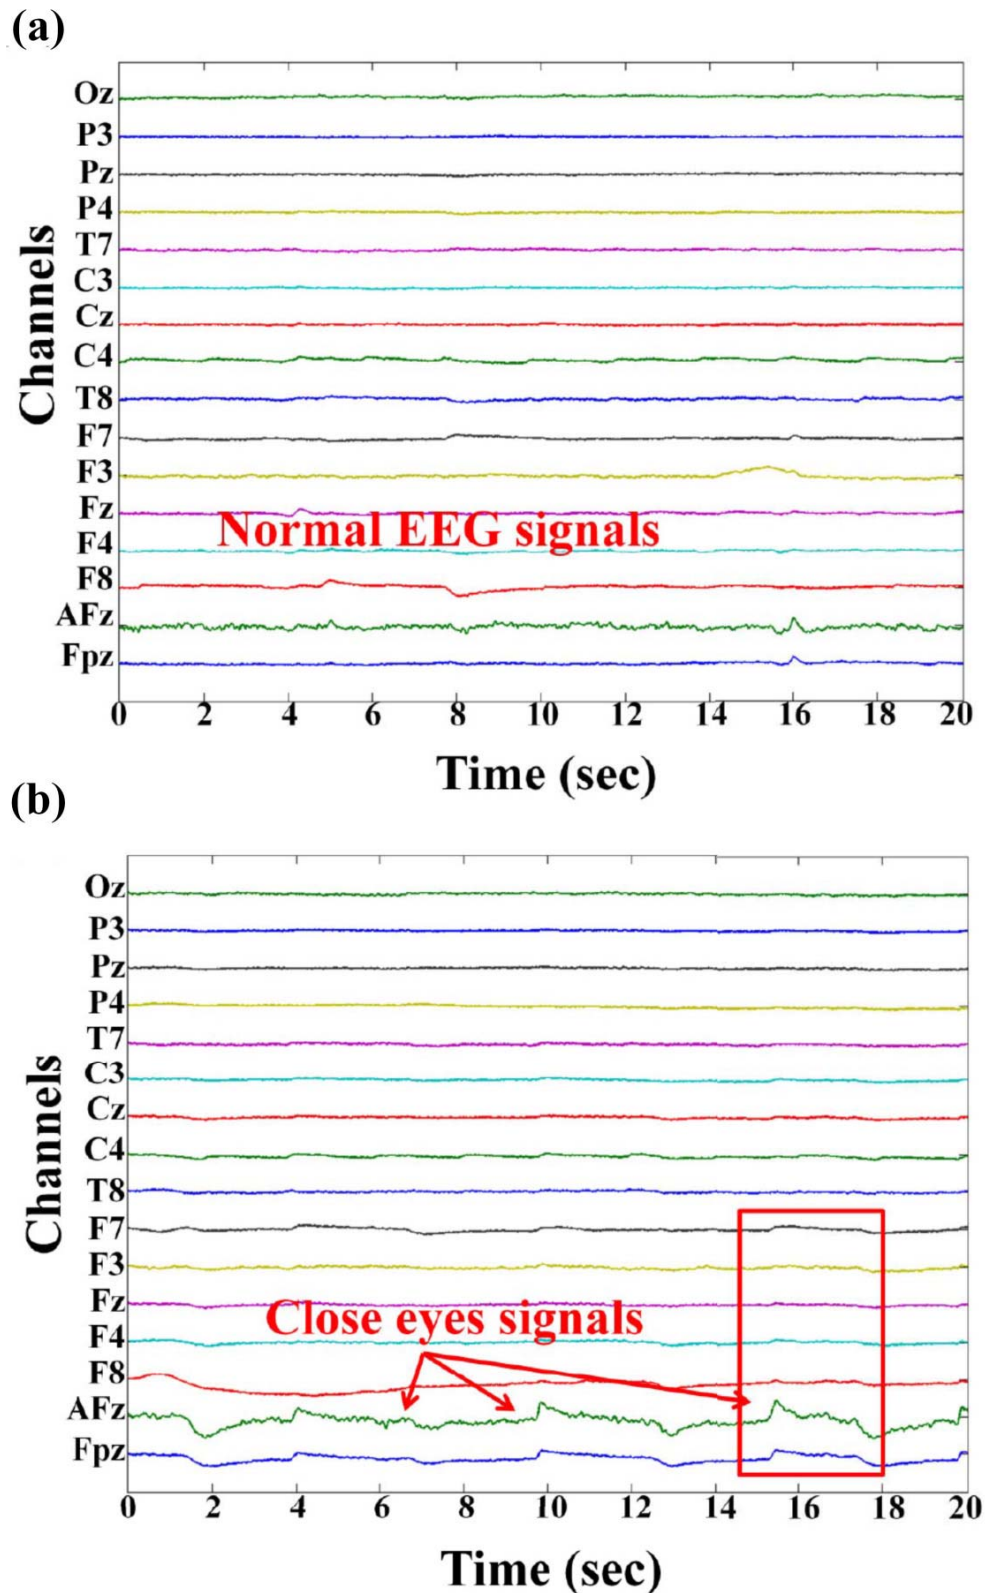


Fig. 6. 16-channel EEG system was used to measure EEG signals from hairy sites using the dry sensors. The data show measurements of (a) normal EEG signals and (b) EEG signals made with the eyes closed.

typically an irregular surface. The inner layer of the cap holds in place the universal joints that connect to the dry sensors on the scalp. This arrangement provides multiple angles of contact with the scalp surface, thus providing stable EEG signals. The

outer layer of the cap, comprised of elastic fiber and Velcro, provides great flexibility for covering the heads of various users. The 16 dry sensors are located on the cap according to international 10–20 system, as shown in Fig. 1(d), with

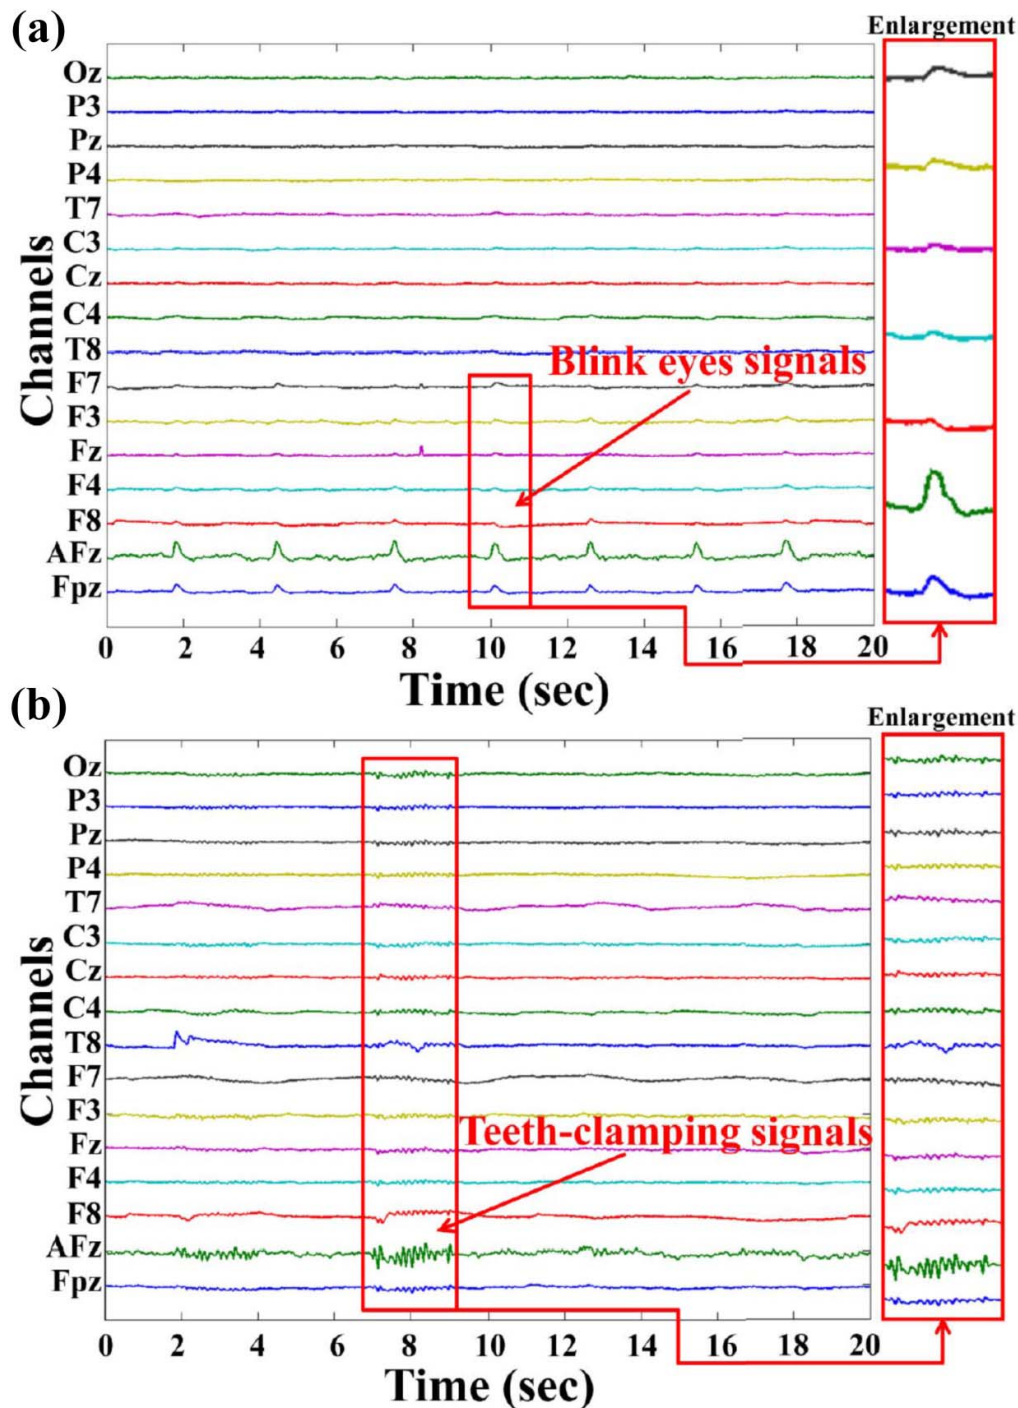


Fig. 7. 16-channel EEG system was used to measure EEG signals on hairy sites using dry sensors. The data show measurements of (a) signals during an eye blink and (b) signals during teeth clenching.

sites Fpz, AFz, F8, F4, Fz, F3, F7, T7, T8, C4, Cz, C3, P4, Pz, P3, and Oz included.

III. RESULTS AND DISCUSSION

The experiments presented here consisted of three major stages. In the first stage, a validation experiment was used to verify the signal quality, as shown in Fig. 4. EEG data were prerecorded using a conventional EEG electrode with a conductive gel. These data were fed into a programmable function generator and passed through a voltage divider, thus

generating simulated human EEG signals. The simulated EEG signals were then fed to a dry electrode, and the output data of the dry electrode were recorded. prerecorded data were used to provide a set of standard EEG patterns for repeated experiments so that the performance of the dry electrodes could be objectively evaluated [9], [36], [38]. Therefore, the physiological meaning of the prerecorded EEG data was not interpreted except to validate the proposed dry sensors. The aim of this validation process was to identify any distortion caused by the dry EEG sensor during EEG measurements.

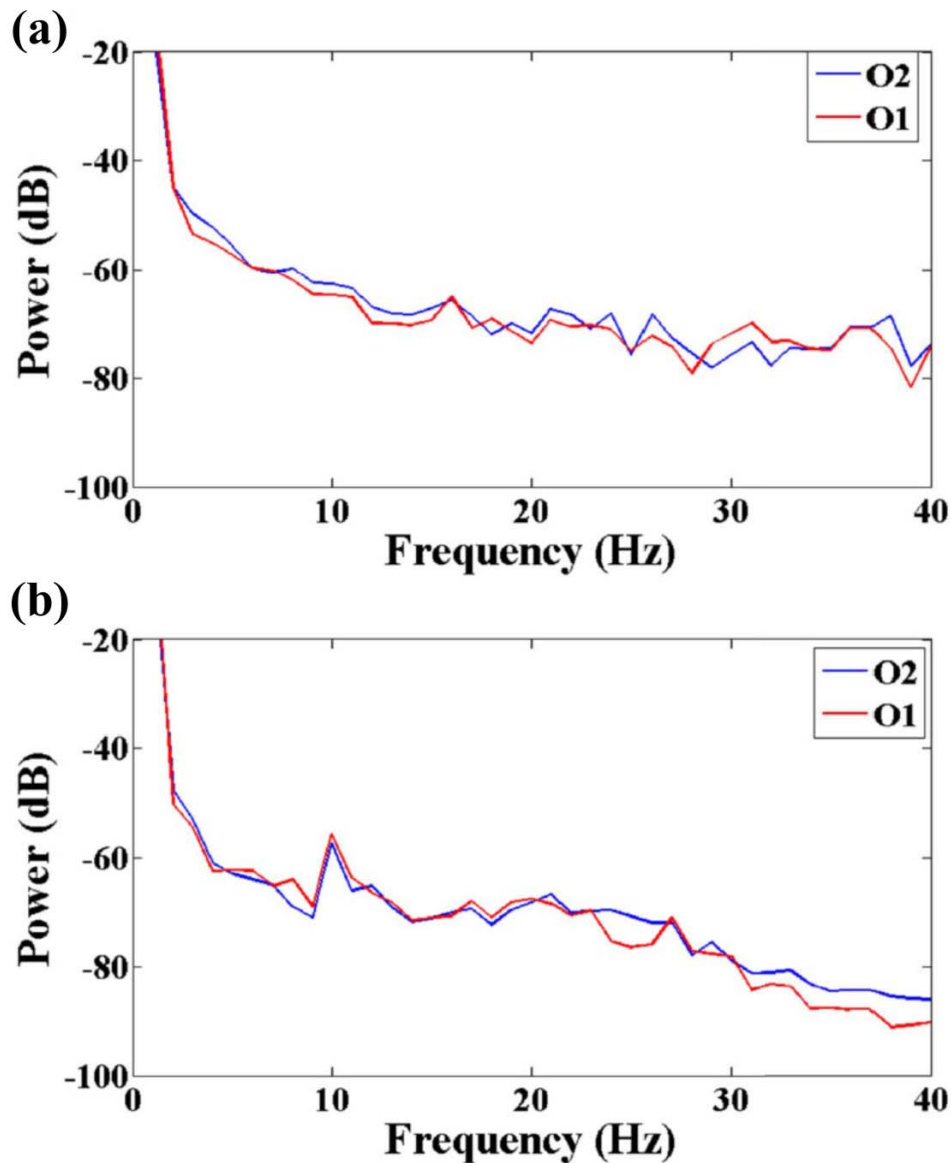


Fig. 8. Results showing the difference between the normal state and the eyes closed state. (a) Subject at rest, showing normal EEG signals from the O1 and O2 channels. (b) Subject with the eyes closed, showing alpha activity in the EEG signal measured from the O1 and O2 channels.

In the second stage, a user sat comfortably in front of a monitor wearing both dry and wet sensor simultaneously. The correlation between the conventional wet EEG electrode and the dry EEG sensor was investigated. Finally, after demonstrating the precision of the signals measured by the dry EEG sensors through the circuit, the newly developed wireless and wearable EEG cap with 16 dry sensors was used to measure a normal EEG, an EEG with the eyes closed, an EEG during an eye blink, and an EEG during teeth clenching, without the use of the conductive gels or skin preparation.

Fig. 4 shows the design of the validation experiment to test the signal quality of the dry sensors. EEG signals were prerecorded using wet electrodes as described above and then transmitted to the data acquisition device. The secondary EEG signals that were recorded by the dry sensors were also transmitted, and the correlation between the signals from the dry and wet sensors was determined. The prerecorded EEG

signals and the signals from the dry EEG sensor were highly correlated at 96.83%.

Fig. 5(a) shows the results of the simultaneous EEG measurements made using both dry and wet sensors located on the forehead (site Fp1). The EEG signals recorded by the wet and dry sensors were highly correlated at 95.53%. In addition to this correlation, the data show that the signal quality from the dry sensor and readout circuit was stable and reliable compared to the wet sensor. Fig. 5(b) shows the results of EEG measurements made using the wet and dry sensors on a hairy site (P3). The correlation of 92.88% on a hairy site is significant.

According to these experimental results, the 16-channel dry sensor system described here can be used for measuring EEG signals with high signal quality, especially on hairy sites. We next measured a series of EEG signals: normal signals, eye-blink signals, signals with the eyes closed, and signals

due to teeth clenching. The normal EEG signals that were measured by the proposed system are shown in Fig. 6(a). The EEG signals could be observed from frontal (i.e., Fpz, AFz, F8, F4, Fz, F3, and F7), temporal (i.e., T7 and T8), central (i.e., C4, Cz, and C3), parietal (i.e., P4, Pz, and P3), and occipital (i.e., Oz) brain regions. Due to the scaling of the plot in the figure, the signal variations appear relatively small, but the raw EEG data were clear and reliable. EEG signals with the eyes closed were also measured by the proposed system, as shown in Fig. 6(b), and were detectable at the frontal sites (i.e., Fpz, AFz, F8, F4, Fz, F3, and F7). In this measurement, the alpha wave was larger. Thus, the signals obtained from the Fpz, AFz, F8, F4, Fz, F3, and F7 sites were more significant than those obtained from the temporal (i.e., T7 and T8), central (i.e., C4, Cz, and C3), parietal (i.e., P4, Pz, and P3), and occipital (i.e., Oz) areas. Fig. 7(a) shows the 16-channel EEG-system measurement of signals during an eye blink. Because the motion of blinking occurs physically near the frontal area, the signals from blinking eyes are significant in the frontal zone (i.e., Fpz, AFz, F8, F4, Fz, F3, and F7). Therefore, during an eye blink, the signals were more obvious on the frontal site relative to other sites (i.e., central, temporal, parietal, and occipital). Fig. 7(b) shows the signal due to teeth clenching, during which the whole head (i.e., frontal, central, temporal, parietal, and occipital) had significant signal variations. Fig. 8(a) and (b) shows the power spectra of the EEG data collected by the dry sensors in this paper, showing characteristic low frequency bands (1–30 Hz). The EEG activity from a subject at rest [Fig. 8(a)] shows the activated reactions caused by holding the eyes open for a few seconds. Because the general alpha frequency band of the EEG signal is distributed between 8 and 12 Hz, the experimental results in Fig. 8(b) fit the trend in the alpha domain.

Here, we have shown positive results from measuring EEG signals with the proposed system and its dry sensors. Our experimental results have shown that dry sensors are capable of recording EEG signals via the EEG measurement system. The signal correlation between measurements performed with dry and wet sensors at the same locations was high. These results are significant with respect to the EEG measurement system because the dry sensors can be utilized without using conductive gel on hairy sites. In addition, these sensors can effectively acquire EEG signals (i.e., normal, closed eyes, blinking, and teeth-clenching signals) in frontal (i.e., Fpz, AFz, F8, F4, Fz, F3, and F7), temporal (i.e., T7 and T8), central (i.e., C4, Cz, and C3), parietal (i.e., P4, Pz, and P3), and occipital (i.e., Oz) areas. In contrast to traditional EEG measurement systems, the use of dry sensors allows users to feel more comfortable and experiments to be performed more quickly.

IV. CONCLUSION

In this paper, a wearable EEG system with dry spring-loaded sensors is proposed to transfer the EEG signals wirelessly to the computer. The developed system contains a size-adjustable soft cap, dry spring-loaded sensors, and a 16-channel acquisition circuit. The experimental results show that the proposed EEG measurement system with dry sensors can provide good

signal quality on hairy sites compared to conventional wet sensors. Unlike the conventional system with wet sensors, the proposed system can be used to measure EEG signals without the use of conductive gel and skin preparation processes. Due to the soft substrate in the dry sensors and the spring-loaded probes, the design ensures that the dry sensors fit on the scalp tightly. The soft cap is suitable for different head sizes (i.e., small, medium, or large) for basic cognitive experiments. The quality of the EEG signal measured with the dry sensors approached that of the signal quality from the wet sensors. Thus, researchers can use the EEG system with dry sensors developed here to reliably investigate human cognitive states in real-life conditions.

ACKNOWLEDGMENT

This work was supported in part by the UST-UCSD International Center of Excellence in Advanced Bio-engineering sponsored by the Taiwan National Science Council I-RiCE Program under Grant Number: NSC 102-2911-I-009-101, in part by NSC-NSC 102-2220-E-009-041 and NSC 102-2627-E-009-002, in part by the Aiming for the Top University Plan, under Contract 103W963.

REFERENCES

- [1] L. D. Liao, C. T. Lin, Y. Y. Shih, T. Q. Duong, H. Y. Lai, P. H. Wang, *et al.*, "Transcranial imaging of functional cerebral hemodynamic changes in single blood vessels using in vivo photoacoustic microscopy," *J. Cereb. Blood Flow Metab.*, vol. 32, no. 6, pp. 938–951, Apr. 2012.
- [2] L.-D. Liao, M.-L. Li, H.-Y. Lai, Y.-Y. I. Shih, Y.-C. Lo, S. Tsang, *et al.*, "Imaging brain hemodynamic changes during rat forepaw electrical stimulation using functional photoacoustic microscopy," *Neuroimage*, vol. 52, no. 2, pp. 562–570, 2010.
- [3] L.-D. Liao, C.-T. Lin, Y.-Y. I. Shih, H.-Y. Lai, W.-T. Zhao, T. Q. Duong, *et al.*, "Investigation of the cerebral hemodynamic response function in single blood vessels by functional photoacoustic microscopy," *J. Biomed. Opt.*, vol. 17, no. 6, pp. 061210-1–061210-10, 2012.
- [4] C. Miniussi and G. Thut, "Combining TMS and EEG offers new prospects in cognitive neuroscience," *Brain Topogr.*, vol. 22, pp. 249–256, Jan. 2010.
- [5] N. Srinivasan, "Cognitive neuroscience of creativity: EEG based approaches," *Methods*, vol. 42, pp. 109–116, May 2007.
- [6] L.-D. Liao and C.-T. Lin, "Novel trends in biosensors used for electroencephalography measurements in neurocognitive engineering applications," *J. Neurosci. Neuroeng.*, vol. 1, no. 1, pp. 32–41, 2012.
- [7] S. Machado, F. Araujo, F. Paes, B. Velasques, M. Cunha, H. Budde, *et al.*, "EEG-based brain-computer interfaces: An overview of basic concepts and clinical applications in neurorehabilitation," *Rev. Neurosci.*, vol. 21, no. 6, pp. 451–468, 2010.
- [8] M. B. Shulman, "The clinical applications of EEG: Origins," *Epilepsy Behavior*, vol. 3, pp. 393–394, Aug. 2002.
- [9] L. D. Liao, C. T. Lin, K. McDowell, A. E. Wickenden, K. Gramann, T. P. Jung, *et al.*, "Biosensor technologies for augmented brain-computer interfaces in the next decades," *Proc. IEEE (Special Centennial Issue)*, vol. 100, pp. 1553–1566, May 2012.
- [10] C. T. Lin, S. H. Liu, J. J. Wang, and Z. C. Wen, "Reduction of interference in oscillometric arterial blood pressure measurement using fuzzy logic," *IEEE Trans. Biomed. Eng.*, vol. 50, no. 4, pp. 432–441, Apr. 2003.
- [11] C. J. Lin, C. H. Chen, and C. T. Lin, "A hybrid of cooperative particle swarm optimization and cultural algorithm for neural fuzzy networks and its prediction applications," *IEEE Trans. Syst., Man, Cybern. C, Appl. Rev.*, vol. 39, no. 1, pp. 55–68, Jan. 2009.
- [12] S. Makeig, C. Kothe, T. Mullen, N. Bigdely-Shamlo, Z. Zhilin, and K. Kreutz-Delgado, "Evolving signal processing for brain-computer interfaces," *Proc. IEEE (Special Centennial Issue)*, vol. 100, pp. 1567–1584, May 2012.
- [13] T. O. Zander, M. Lehne, K. Ihme, S. Jatzev, J. Correia, C. Kothe, *et al.*, "A dry EEG-system for scientific research and brain-computer interfaces," *Front. Neurosci.*, vol. 5, pp. 1–10, May 2011.

- [14] N. V. Thakor, "Biopotentials and electro-physiology measurement," in *The Measurement, Instrumentation, Sensors Handbook*. Boca Raton, FL, USA: CRC Press, 1999, pp. 74-1-74-9.
- [15] R. Rao and R. Scherer, "Brain-computer interfacing [in the spotlight]," *IEEE Signal Process. Mag.*, vol. 27, no. 4, pp. 152-150, Jul. 2010.
- [16] C. Schuster, R. Hilfiker, O. Amft, A. Scheidhauer, B. Andrews, J. Butler, U. Kischka, et al., "Best practice for motor imagery: A systematic literature review on motor imagery training elements in five different disciplines," *BMC Med.*, vol. 9, pp. 75-109, Jun. 2011.
- [17] W.-Y. Hsu, "EEG-based motor imagery classification using enhanced active segment selection and adaptive classifier," *Comput. Biol. Med.*, vol. 41, pp. 633-639, Aug. 2011.
- [18] M. V. Stecklow, A. F. Infantosi, and M. Cagy, "EEG changes during sequences of visual and kinesthetic motor imagery," *Arq. Neuro-Psiquiatr.*, vol. 68, pp. 556-561, Aug. 2010.
- [19] N. Pouratian, "Editorial note on: On the feasibility of using motor imagery EEG-based brain-computer interface in chronic tetraplegics for assistive robotic arm control: A clinical test and long-term post trial follow-up," *Spinal Cord*, vol. 50, p. 716, Mar. 2012.
- [20] S. Hu, R. L. Bowlds, Y. Gu, and X. Yu, "Pulse wave sensor for non-intrusive driver's drowsiness detection," in *Proc. Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.*, Sep. 2009, pp. 2312-2315.
- [21] C. T. Lin, Y. C. Chen, T. Y. Huang, T. T. Chiu, L. W. Ko, S. F. Liang, et al., "Development of wireless brain computer interface with embedded multitask scheduling and its application on real-time driver's drowsiness detection and warning," *IEEE Trans. Biomed. Eng.*, vol. 55, no. 5, pp. 1582-1591, May 2008.
- [22] K. Marcellis, M. Verduyssen, E. Nicu, I. Naert, and M. Quirynen, "Sleeping vs. loaded implants, long-term observations via a retrospective analysis," *Clin. Oral Implants Res.*, vol. 23, pp. 1118-1122, Nov. 2011.
- [23] B. T. Brett, K. E. Berquam-Vrieze, K. Nannapaneni, J. Huang, T. E. Scheetz, and A. J. Dupuy, "Novel molecular and computational methods improve the accuracy of insertion site analysis in sleeping beauty-induced tumors," *Public Library Sci. One*, vol. 6, pp. 1-11, Sep. 2011.
- [24] R. Matthews, P. J. Turner, N. J. McDonald, K. Ermolaev, T. M. Manus, R. A. Shelby, et al., "Real time workload classification from an ambulatory wireless EEG system using hybrid EEG electrodes," in *Proc. 30th Annu. Int. Conf. IEEE EMBS*, Aug. 2008, pp. 5871-5875.
- [25] R. Matthews, N. McDonald, H. Anumula, J. Woodward, P. Turner, M. Steindorf, et al., "Novel hybrid bioelectrodes for ambulatory zero-prep EEG measurements using multi-channel wireless EEG system," in *Foundations of Augmented Cognition* (Lecture Notes in Computer Science), vol. 4565. New York, NY, USA: Springer-Verlag, 2007, pp. 137-146.
- [26] G. Ruffini, S. Dunne, E. Farrés, J. Marco-Pallarés, C. Ray, E. Mendoza, et al., "A dry electrophysiology electrode using CNT arrays," *Sens. Actuators A, Phys.*, vol. 132, pp. 34-41, Apr. 2006.
- [27] Y. S. Kim, H. J. Baek, J. S. Kim, H. B. Lee, J. M. Choi, and K. S. Park, "Helmet-based physiological signal monitoring system," *Eur. J. Appl. Physiol.*, vol. 105, pp. 365-372, Feb. 2009.
- [28] C. Fonseca, J. P. S. Cunha, R. E. Martins, V. M. Ferreira, J. P. Marques de Sa, M. A. Barbosa, et al., "A novel dry active electrode for EEG recording," *IEEE Trans. Biomed. Eng.*, vol. 54, no. 1, pp. 162-165, Jan. 2007.
- [29] P. Griss, H. K. Tolvanen-Laakso, P. Merilainen, and G. Stemme, "Characterization of micromachined spiked biopotential electrodes," *IEEE Trans. Biomed. Eng.*, vol. 49, no. 6, pp. 597-604, Jun. 2002.
- [30] P. Griss, P. Enoksson, H. K. Tolvanen-Laakso, P. Merilainen, S. Ollmar, and G. Stemme, "Micromachined electrodes for biopotential measurements," *J. Microelectromech. Syst.*, vol. 10, pp. 10-16, Mar. 2001.
- [31] L.-D. Liao, P. C.-P. Chao, Y.-H. Chen, C.-T. Lin, L.-W. Ko, H.-H. Lin, et al., "A novel hybrid bioelectrode module for the zero-prep EEG measurements," in *Proc. IEEE Sensors*, Oct. 2009, pp. 939-942.
- [32] J.-C. Chiou, L.-W. Ko, C.-T. Lin, C.-T. Hong, T.-P. Jung, S.-F. Liang, et al., "Using novel MEMS EEG sensors in detecting drowsiness application," in *Proc. IEEE Biomed. Circuits Syst. Conf.*, Nov/Dec. 2006, pp. 33-36.
- [33] L. D. Liao, C. Y. Chen, I. J. Wang, S. F. Chen, S. Y. Li, B. W. Chen, et al., "Gaming control using a wearable and wireless EEG-based brain-computer interface device with novel dry foam-based sensors," *J. Neuroeng. Rehabil.*, vol. 9, pp. 5-15, Jan. 2012.
- [34] C.-T. Lin, L.-D. Liao, Y.-H. Liu, I. J. Wang, B.-S. Lin, and J.-Y. Chang, "Novel dry polymer foam electrodes for long-term EEG measurement," *IEEE Trans. Biomed. Eng.*, vol. 58, no. 5, pp. 1200-1207, May 2011.
- [35] K. Gramann, J. T. Gwin, D. P. Ferris, K. Oie, T. P. Jung, C. T. Lin, et al., "Cognition in action: Imaging brain/body dynamics in mobile humans," *Rev. Neurosci.*, vol. 22, no. 6, pp. 593-608, 2011.
- [36] L.-D. Liao, I. J. Wang, S.-F. Chen, J.-Y. Chang, and C.-T. Lin, "Design, fabrication and experimental validation of a novel dry-contact sensor for measuring electroencephalography signals without skin preparation," *Sensors*, vol. 11, no. 6, pp. 5819-5834, 2011.
- [37] C. R. Merritt, H. T. Nagle, and E. Grant, "Fabric-based active electrode design and fabrication for health monitoring clothing," *IEEE Trans. Inf. Technol. Biomed.*, vol. 13, no. 2, pp. 274-280, Mar. 2009.
- [38] C.-T. Lin, L.-D. Liao, Y.-H. Liu, I.-J. Wang, B.-S. Lin, and J.-Y. Chang, "Novel dry polymer foam electrodes for long-term EEG measurement," *IEEE Trans. Biomed. Eng.*, vol. 58, no. 5, pp. 1200-1207, May 2011.
- [39] W. O. Tatum, B. A. Dworetzky, and D. L. Schomer, "Artifact and recording concepts in EEG," *J. Clin. Neurophysiol.*, vol. 28, pp. 252-263, Jun. 2011.
- [40] W. O. Tatum, B. A. Dworetzky, W. D. Freeman, and D. L. Schomer, "Artifact: Recording EEG in special care units," *J. Clin. Neurophysiol.*, vol. 28, pp. 264-277, Jun. 2011.
- [41] R. L. Boylestad and L. Nashelsky, *Electronic Devices and Circuit Theory*, 10th ed. Upper Saddle River, NJ, USA: Prentice-Hall, 2009.
- [42] D. A. Neamen, *Microelectronics: Circuit Analysis and Design*, 3rd ed. New York, NY, USA: McGraw-Hill, 2007.
- [43] R. W. Homan, J. Herman, and P. Purdy, "Cerebral location of international 10-20 system electrode placement," *Electroencephalogr. Clin. Neurophysiol.*, vol. 66, pp. 376-382, Apr. 1987.



Lun-De Liao received the B.S. degree in mechanical engineering from Chung Yuan Christian University, Zhongli, Taiwan, in 2006, the M.S. degree in engineering science from National Cheng-Kung University, Tainan, Taiwan, in 2008, and the Ph.D. degree in electrical engineering from National Chiao-Tung University (NCTU), Hsinchu, Taiwan, in 2012.

He was a Research Fellow with the Brain Research Center, NCTU. He is currently a Research Scientist with the Singapore Institute for Neurotechnology, National University of Singapore, Singapore. He is

the author of *Relativistic Molecular Dynamics Simulation of Ultrafast Laser Ablation* (VDM Verlag, 2008). He has published over 30 peer-reviewed SCI journal papers. His current research interests include biomedical optics imaging, advanced sensing techniques, neuroimaging, and cognitive neuroscience.

Dr. Liao was a recipient of the 2005 Best Paper Award from the National Society of Engineers, Taiwan, the 2005 Best Paper Award from the College of Engineering at Chung Yuan Christian University, the 2006 Best Paper Award from the Department of Mechanical Engineering, Chung Yuan Christian University, the 2005 and 2006 Outstanding Course Score Scholarship from Chung Yuan Christian University, the 2006 AUO Award, the 2006 Acer Long-Term 3rd-Prize Award, the 2006 North-Eastern Flat-Panel Displays 1st-Prize Award, the 2007 Top Research Paper Award of the Year selected from the *SPIE* journal selected, the 2007 MekTec 3rd-Prize Award, the 2007 Acer Long-Term 2nd-Prize Award, the 2009 SID Travel Fellowship, the 2009 IEEE Intermag Travel Fellowship, the 2009 Best Paper Award from the Symposium on NanoDevice Technology, the 2010 Honorable Design Award from the National Embedded System Design Contest by Ministry of Education, and the 2010 Best Paper Award from the International Symposium on Biomedical Engineering. In 2011, he received the First Place Young Investigator's Award from the World Association for Chinese Biomedical Engineers for his contributions to medical imaging and bioelectronics domain. He was also selected as an Outstanding Research Award recipient from National Chiao-Tung University, for his outstanding performance during his Ph.D. program. He currently serves as an Editor-in-Chief of the *Journal of Neuroscience and Neuroengineering* and an Associate Editor of the *Advanced Science, Engineering and Medicine*.



Shang-Lin Wu was born in Kaohsiung, Taiwan, in 1987. He received the B.S. and M.S. degrees from the Department of Computer Science and Information Engineering, National Chiayi University, Chiayi, Taiwan, in 2009, and 2011, respectively. He is currently pursuing the Ph.D. degree with the Institute of Electrical Control Engineering, National Chiao-Tung University, Hsinchu, Taiwan.

His current research interests include biomedical signal processing, biofeedback control, and embedded systems.



Chang-Hong Liou was born in Kaohsiung, Taiwan, in 1988. He received the B.S. degree in electronics engineering from the National Changhua University of Education, Changhua, Taiwan, in 2010, and the M.S. degree in electrical control engineering from National Chiao-Tung University, Hsinchu, Taiwan, in 2012.

His current research interests include control engineering, biomedical signal/image processing, brain-computer interfaces, and cognitive neural engineering.



Shao-Wei Lu was born in Taoyuan, Taiwan, in 1980. He received the B.S. degree from the Department of Physics, National Tsing Hua University, Beijing, China, in 2004, and the master's degree from the Institute of Molecular Medicine, National Tsing Hua University in 2007. He is currently pursuing the Ph.D. degree in electrical control engineering with National Chiao-Tung University, Hsinchu, Taiwan.

His current research interests include the information coding of the rabbit retinal ganglion cells.



Shi-An Chen received the Ph.D. degree in electrical and control engineering from National Chiao-Tung University, Hsinchu, Taiwan, in 2011.

He is currently with the Brain Research Center, National Chiao-Tung University, as a Post-Doctoral Researcher. His research focuses on spatial and frequency properties of EEG and cognition state analysis. His current research interests include biomedical signal processing and application of brain-computer interaction.



Li-Wei Ko received the B.S. degree in mathematics from National Chung Cheng University, Chiayi, Taiwan, in 2001, the M.S. degree in educational measurement and statistics from National Taichung University, Taichung, Taiwan, in 2004, and the Ph.D. degrees in electrical engineering from National Chiao-Tung University (NCTU), Hsinchu, Taiwan, in 2007.

He currently is an Assistant Professor with the Department of Biological Science and Technology, and Brain Research Center, NCTU. He is a Visiting

Scholar with the Institute for Neural Computation, University of California, San Diego, CA, USA. His current research interests include EEG signal processing and applying computational intelligence technologies to analyze neural activities associated with human cognitive functions and develop the mobile and wireless brain machine interface in unconstrained actively engaged human subjects in daily life applications, neural networks, neural fuzzy systems, machine learning, brain-computer interface, and computational neuroscience.

Dr. Ko serves as an Associate Editor of the IEEE TRANSACTIONS ON NEURAL NETWORKS AND LEARNING SYSTEMS in the IEEE Computational Intelligence Society (CIS) and the *Journal of Neuroscience and Neuroengineering*. He is a member of the Neural Network Technical Committee and Fuzzy Systems Technical Committee in the IEEE CIS.



Sheng-Fu Chen received the B.S. degree in electronic engineering from Tamkang University, Tamsui, Taiwan, in 1992, and the Ph.D. degree in biomedical engineering from National Yang-Ming University, Taipei, Taiwan, in 2002.

He is currently with the Division of Medical Engineering Research, National Health Research Institutes, Zhunan, Taiwan, as a Research Associate. His current research interests include bioamplifier circuits design, ultrasonic amplifier circuit design, and microcontroller system.



Chin-Teng Lin (F'05) received the B.S. degree in control engineering from National Chiao-Tung University (NCTU), Hsinchu, Taiwan, in 1986, and the M.S.E.E. and Ph.D. degrees in electrical engineering from Purdue University, West Lafayette, IN, USA, in 1989 and 1992, respectively.

He has been with the College of Electrical Engineering and the College of Computer Science, NCTU, since 1992, where he is the Provost and the Lifelong Chair Professor with the Department of Electrical Engineering. He served as the Founding

Dean of the Computer Science College, NCTU, from 2005 to 2007. He authored the textbook entitled *Neural Fuzzy Systems* (Prentice Hall) and *Neural Fuzzy Control Systems with Structure and Parameter Learning* (World Scientific). He has published over 165 journal papers, including over 77 IEEE TRANSACTIONS papers. His current research interests include translational neuroscience, computational intelligent technologies, soft computing, brain-computer interface, smart living technology, intelligent transportation systems, robotics and intelligent sensing, and nano/bioinformation technologies and cognitive science.

Dr. Lin is a member of Tau Beta Pi, Eta Kappa Nu, and Phi Kappa Phi Honorary Societies. He was elevated to IEEE Fellow in 2005 for contributions to biologically inspired information systems. He was honored with Outstanding Electrical and Computer Engineer, Purdue University, in 2011. He was a member of the Board of Governors of the IEEE Systems, Man, Cybernetics Society from 2003 to 2005 and the IEEE Circuit and Systems Society from 2005 to 2008, and is currently an AdCom Member of the IEEE Computational Intelligence Society from 2008 to 2010. He is the IEEE Distinguished Lecturer from 2003 to 2005. He currently serves as an Editor-in-Chief (EIC) of the IEEE TRANSACTIONS ON FUZZY SYSTEMS and Co-EIC of the *Journal of Neuroscience and Neuroengineering*. He was an Associate Editor of the IEEE TRANSACTIONS ON SYSTEMS, MAN, AND CYBERNETICS, PART II. He served as the Deputy EIC of the IEEE TRANSACTIONS ON CIRCUITS AND SYSTEMS, PART II from 2006 to 2007. He is the General Chair of the FUZZ-IEEE 2011, Taipei, and was the Program Chair of the 2006 IEEE International Conference on Systems, Man, and Cybernetics, Taipei. He was the President of the Board of Government of Asia Pacific Neural Networks Assembly from 2004 to 2005. He has received the Outstanding Research Award granted by the National Science Council, Taiwan, in 1997, the Outstanding Professor Award granted by the Chinese Institute of Engineering in 2000, and the 2002 Taiwan Outstanding Information-Technology Expert Award. He was elected to be one of 38th Ten Outstanding Rising Stars in Taiwan in 2000.