

Fig. 3.16 Small signal representation of a common source FET

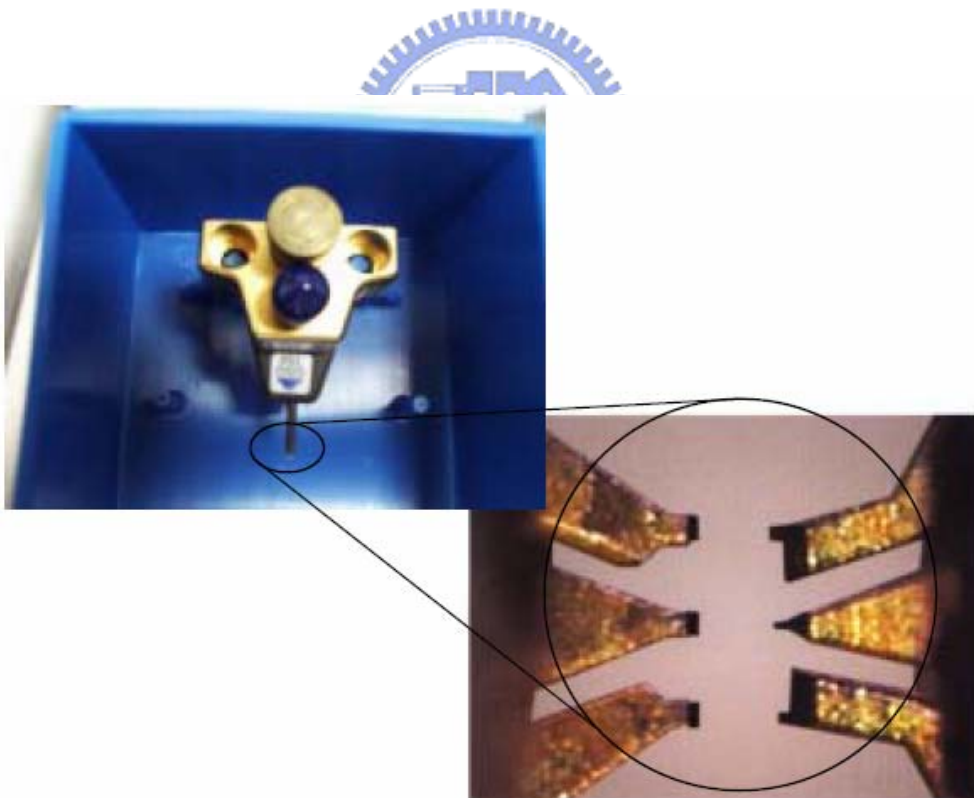


Fig. 3.17 CGS probe tips for the microwave measurement

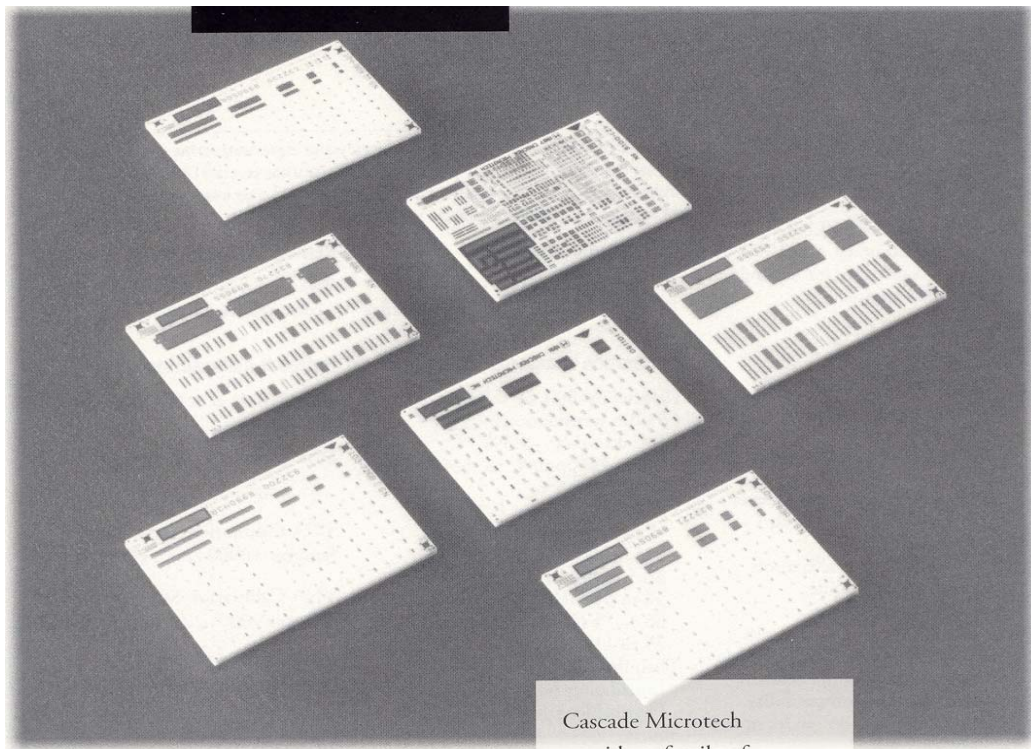


Fig. 3.18 Different ISS substrates for the calibration

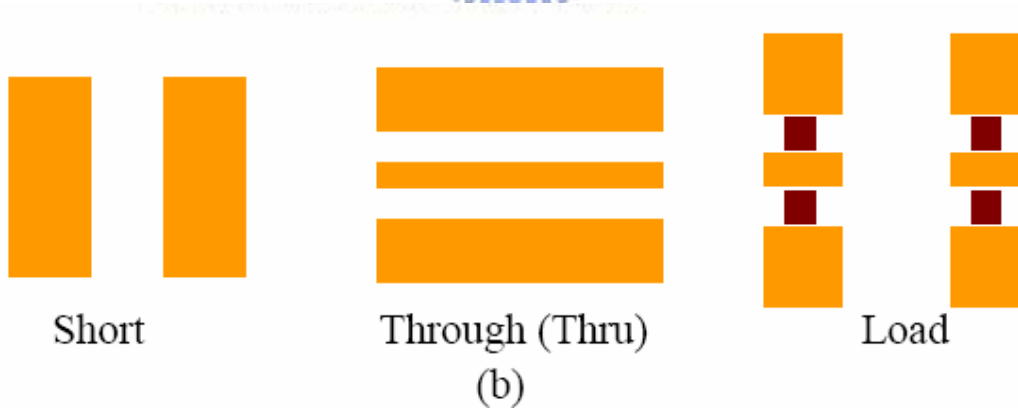


Fig. 3.19 Short, through and loads for the calibration

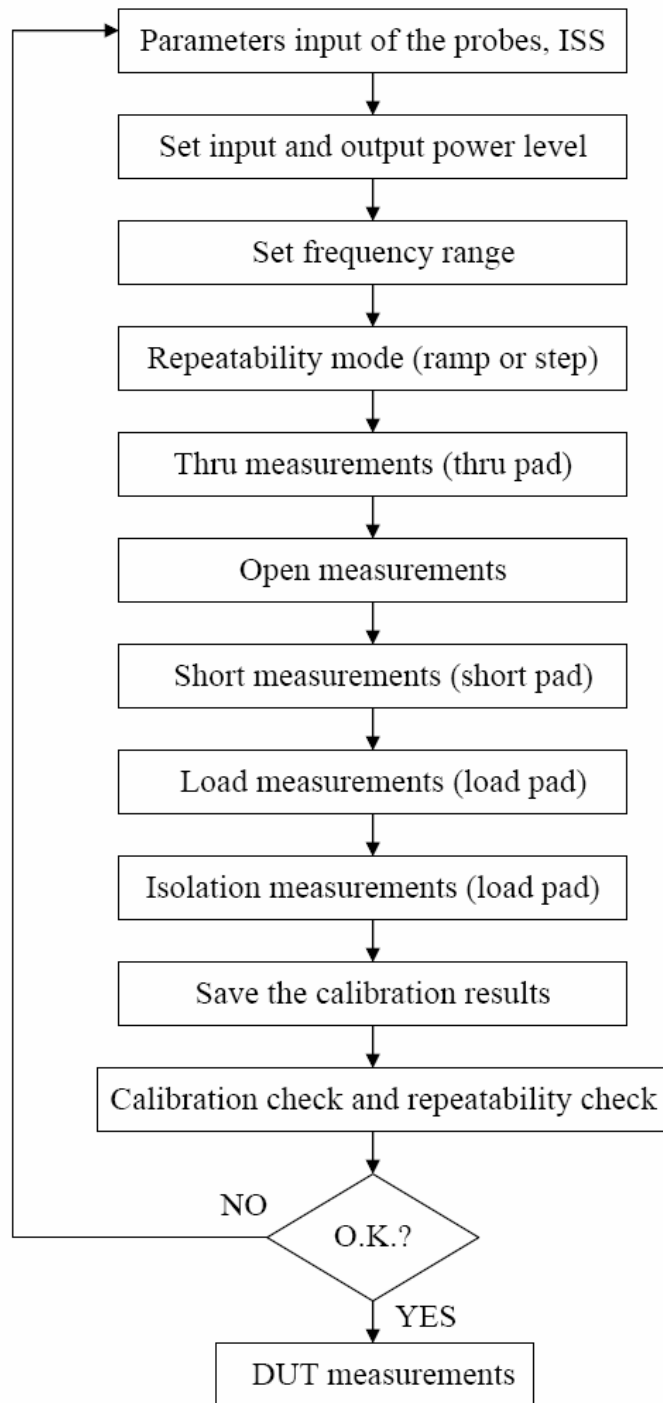


Fig. 3.20 Follow chart for the RF measurement calibration